

Fig. 1

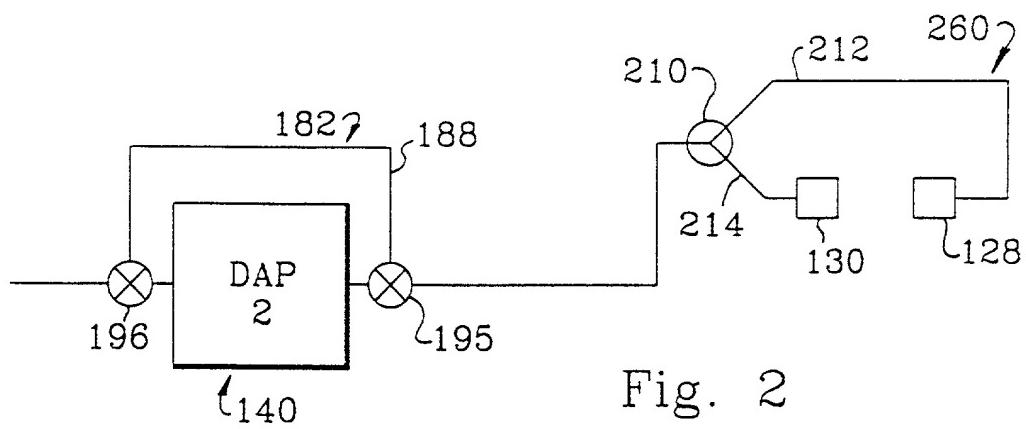


Fig. 2

Fig. 3

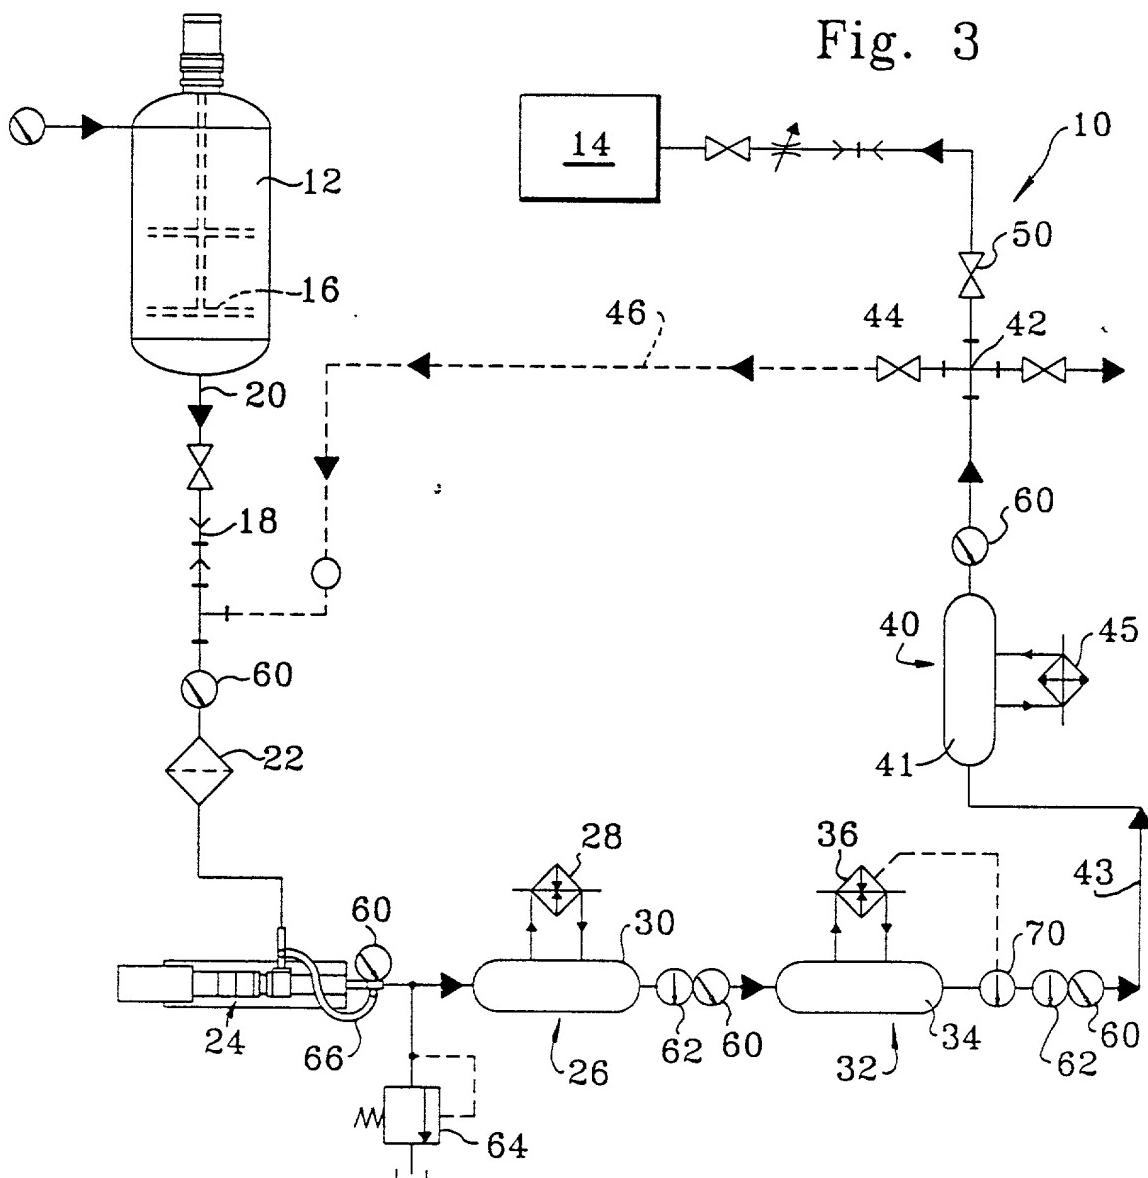


Fig. 4


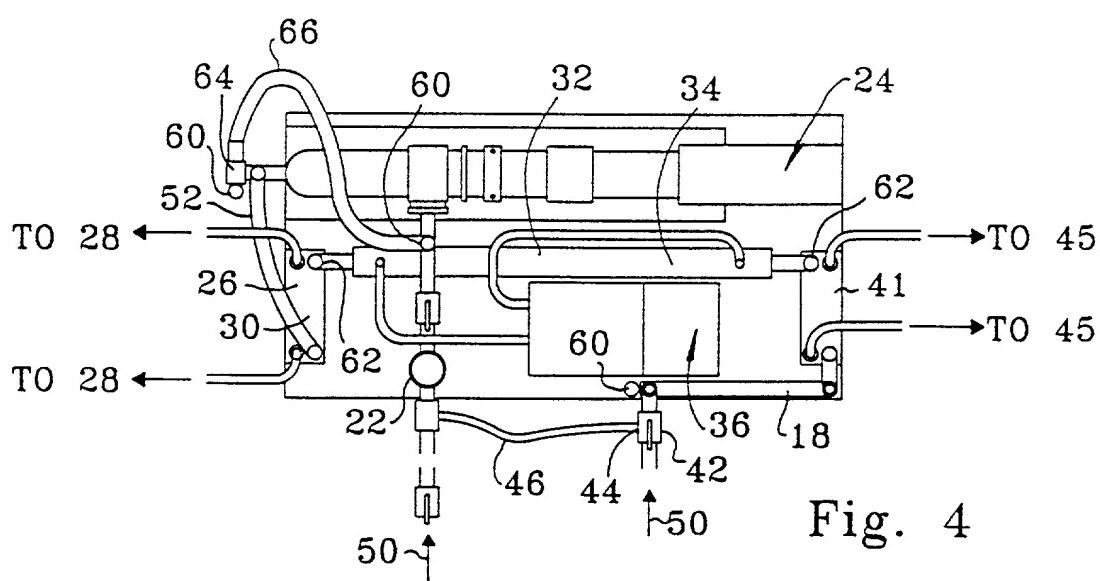


Fig. 5

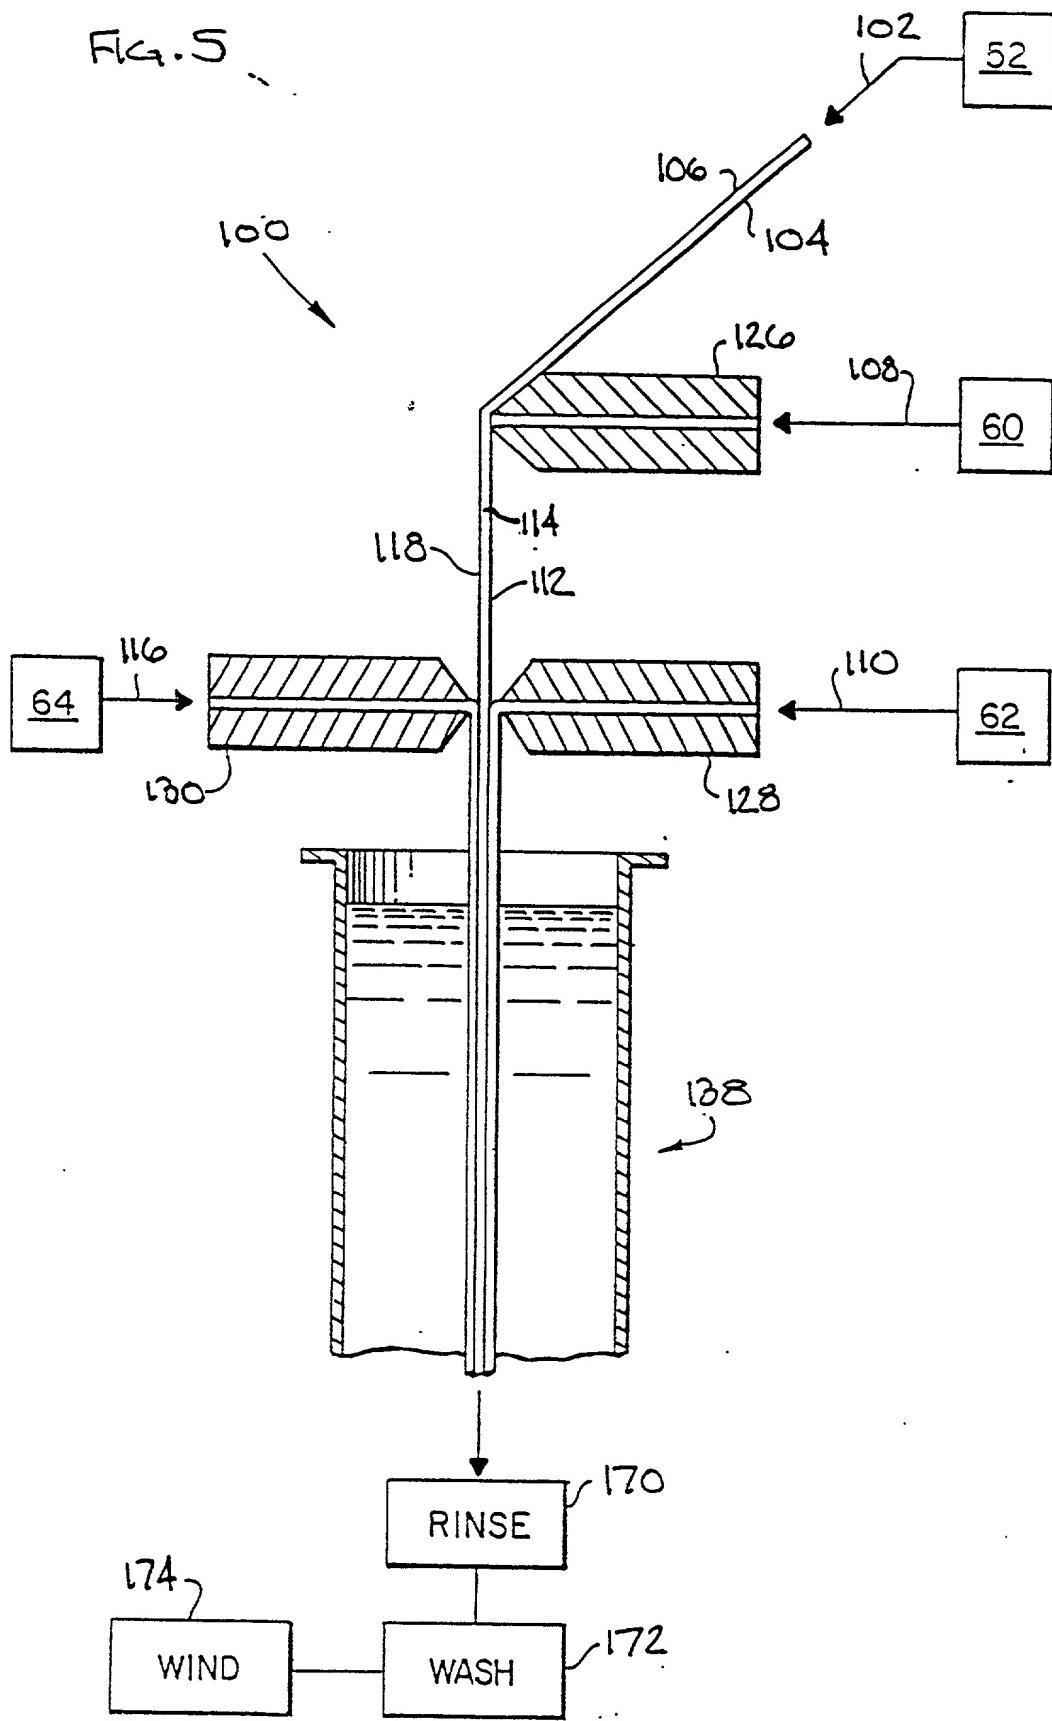

4/14

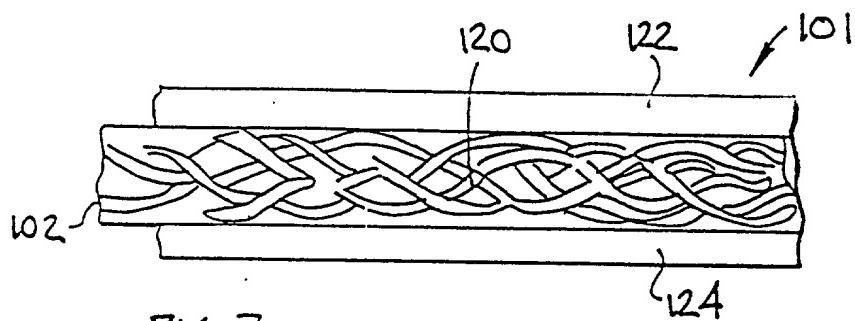


FIG. 7

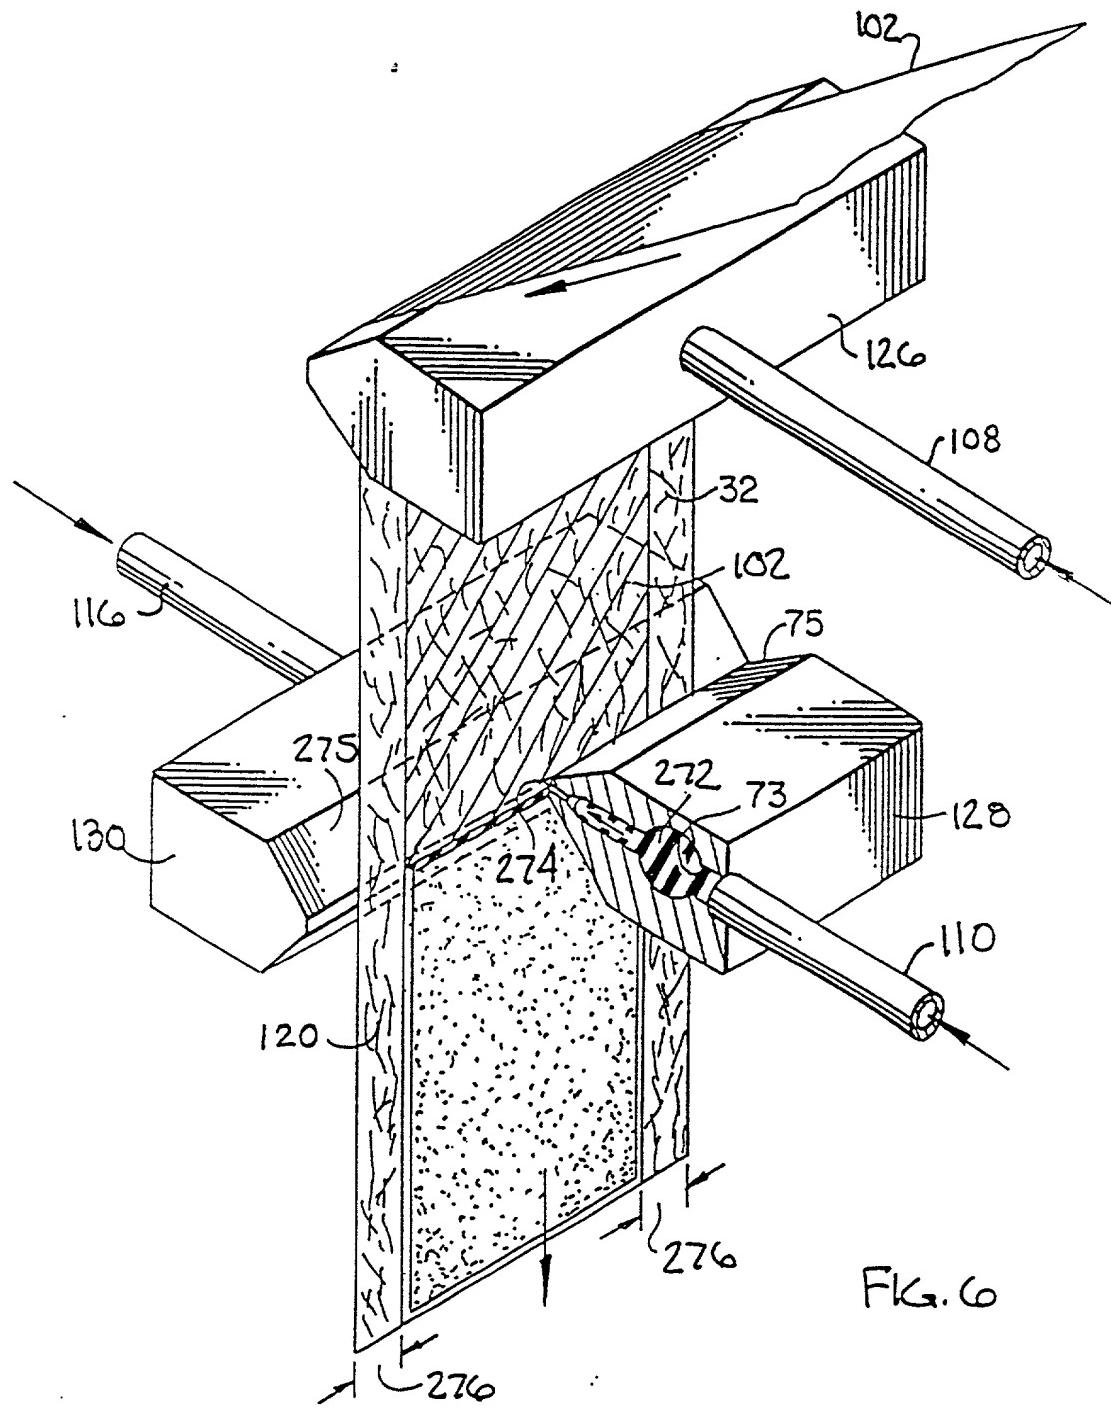


Fig. 6

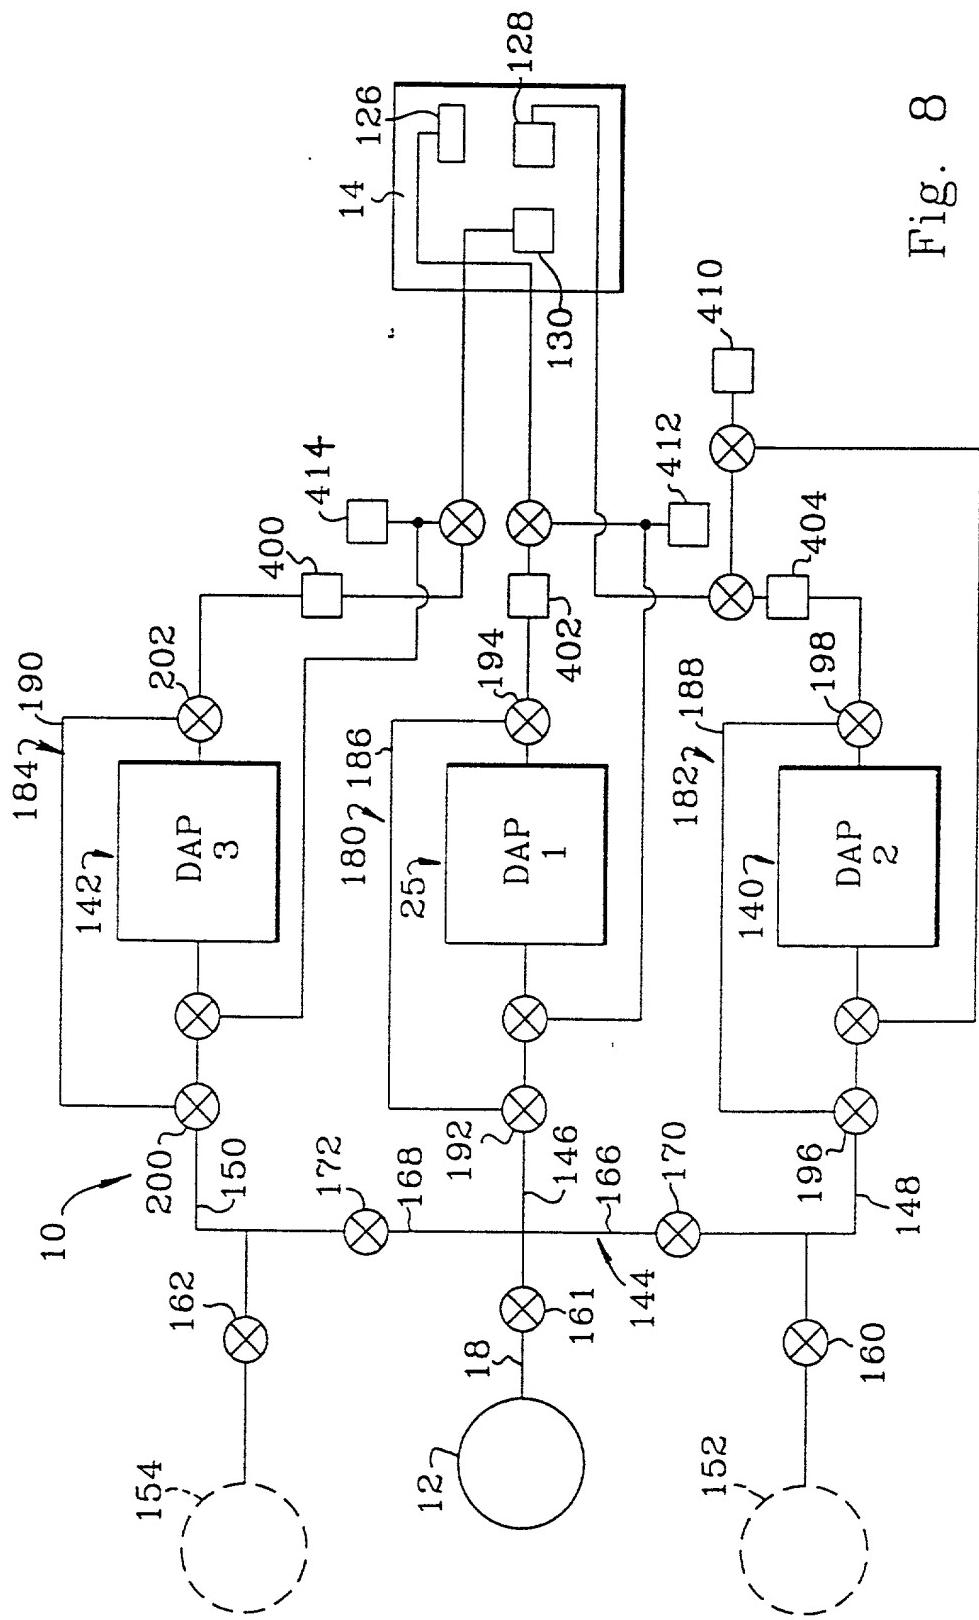


Fig. 8

6/14

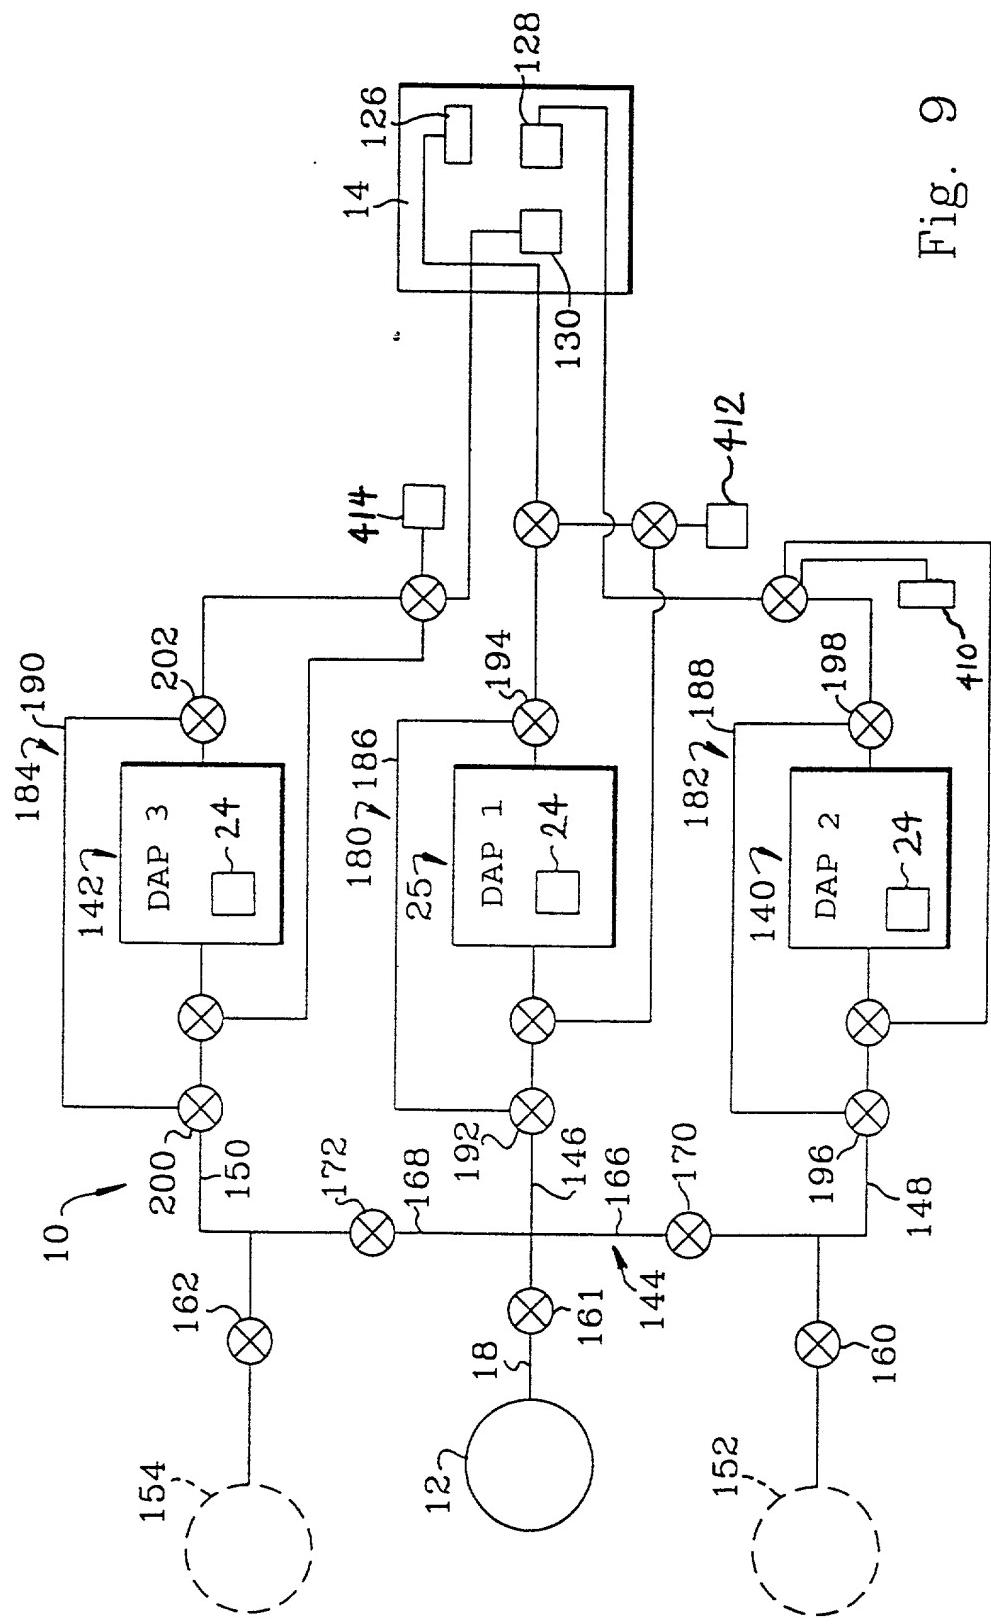


Fig. 9

7/14

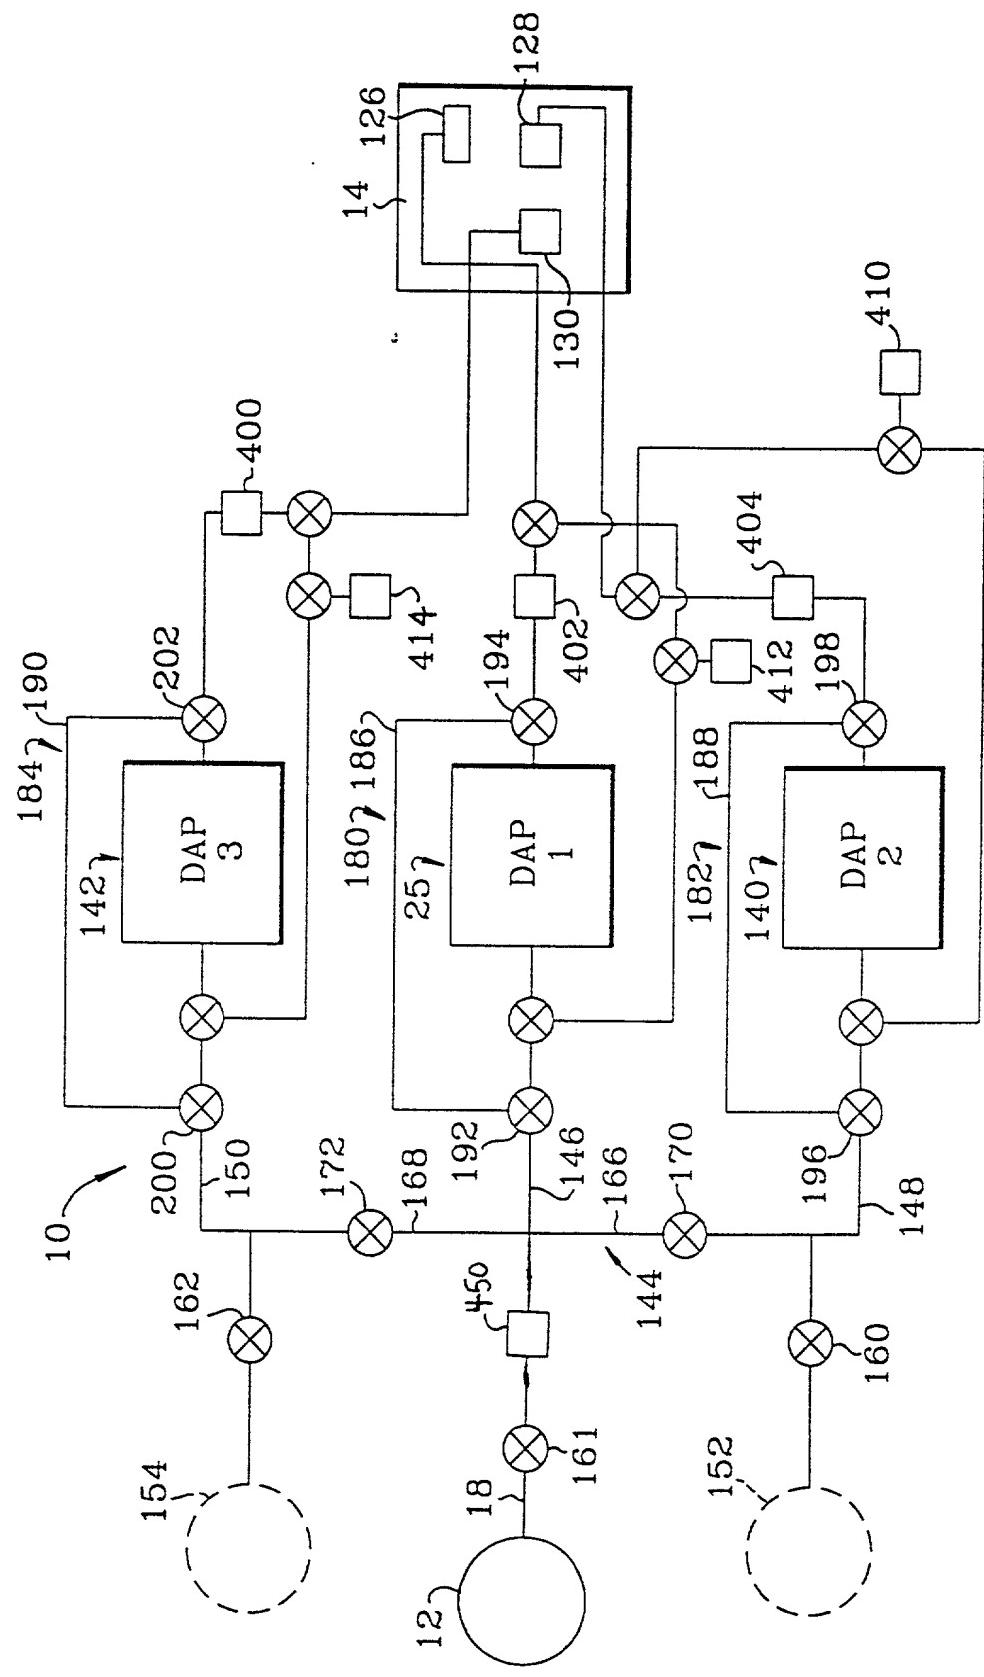


Fig. 10

8/14

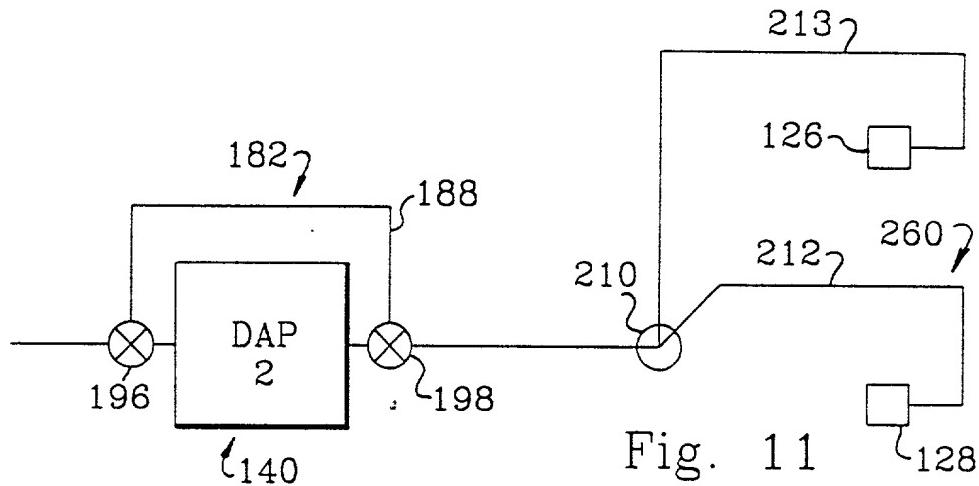


Fig. 11

9/14

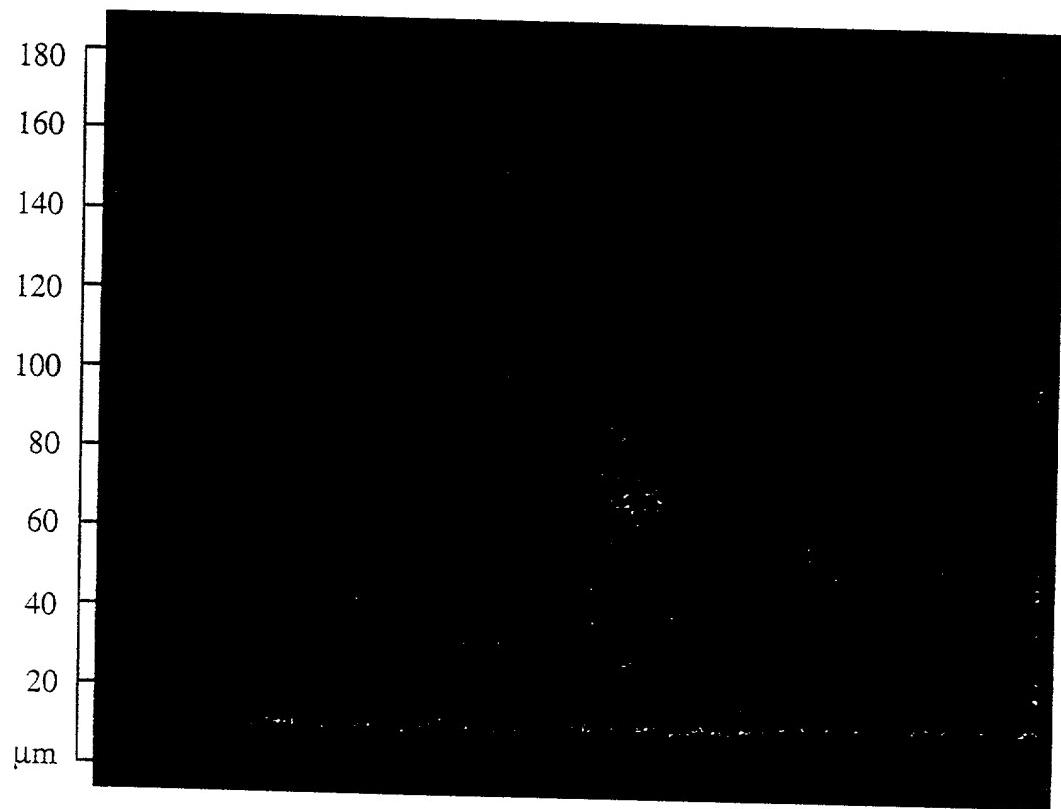


Fig. 12 a

10/14

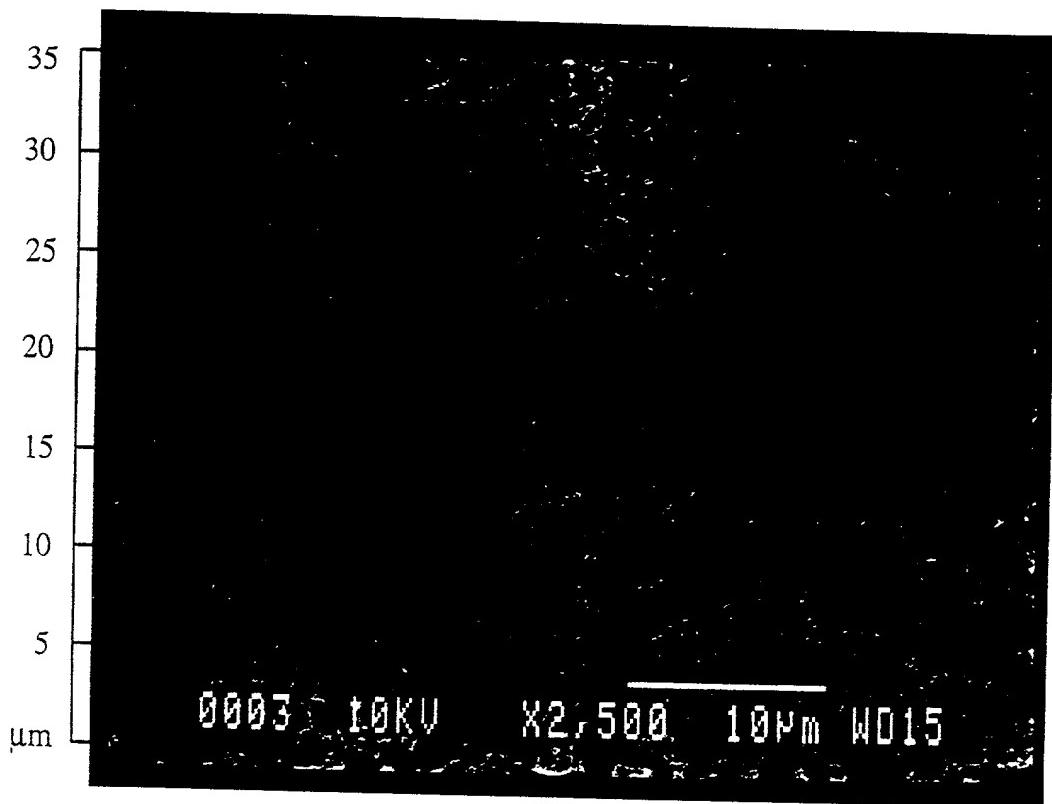


Fig. 12b

11/14

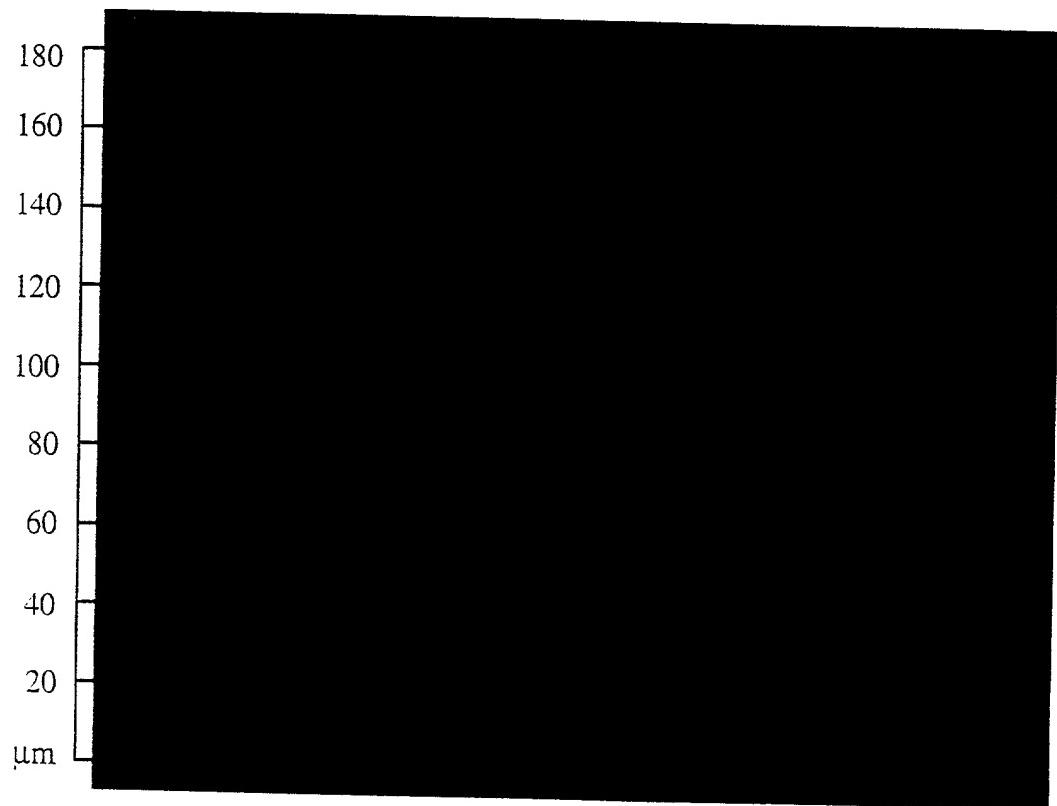


Fig. 13a

12/14

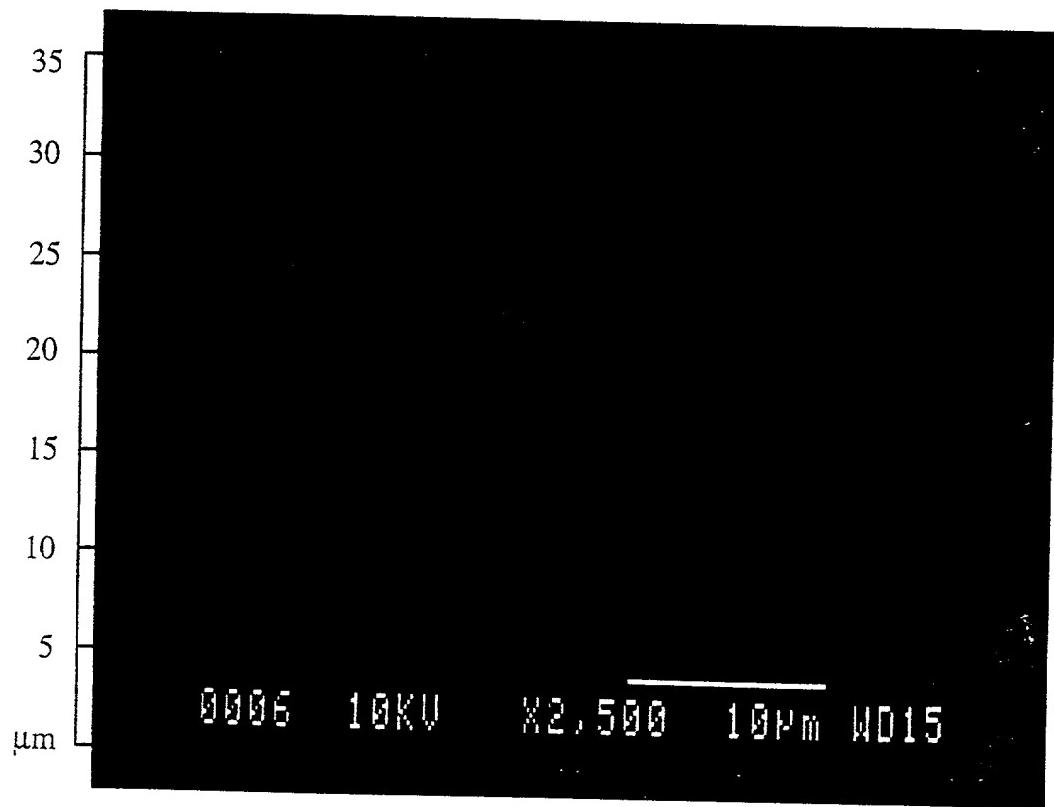


Fig. 13b

13/14

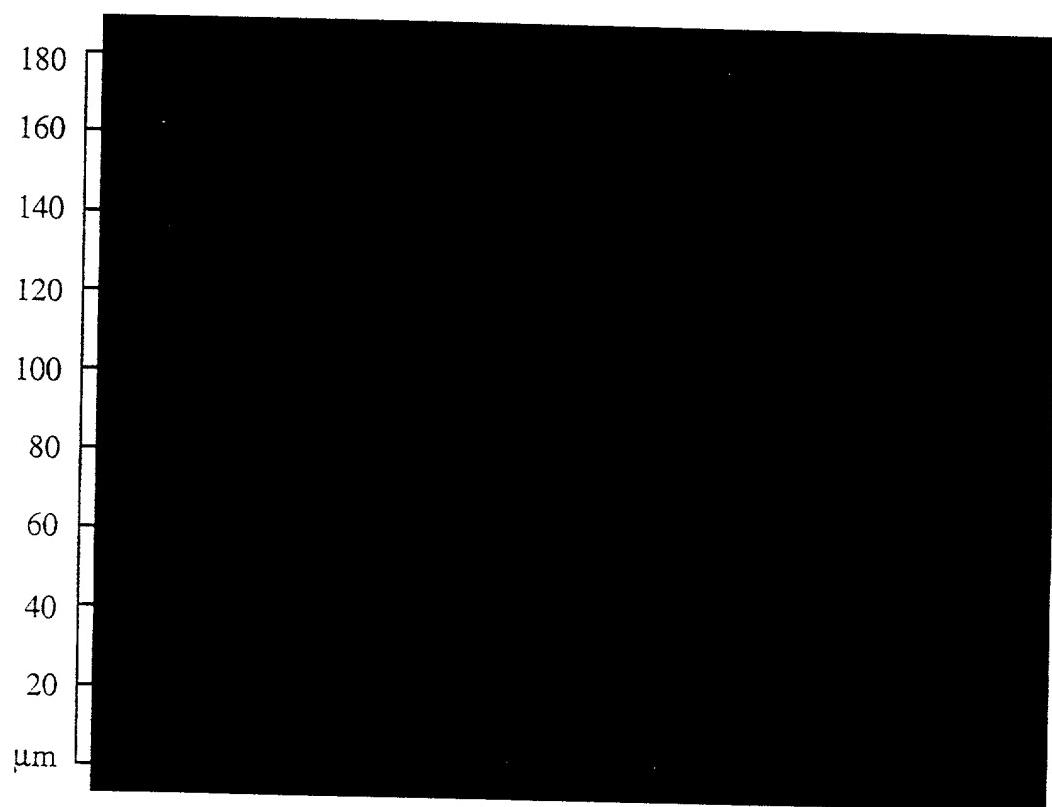


Fig. 14a

14/14

Scanning Electron Micrograph

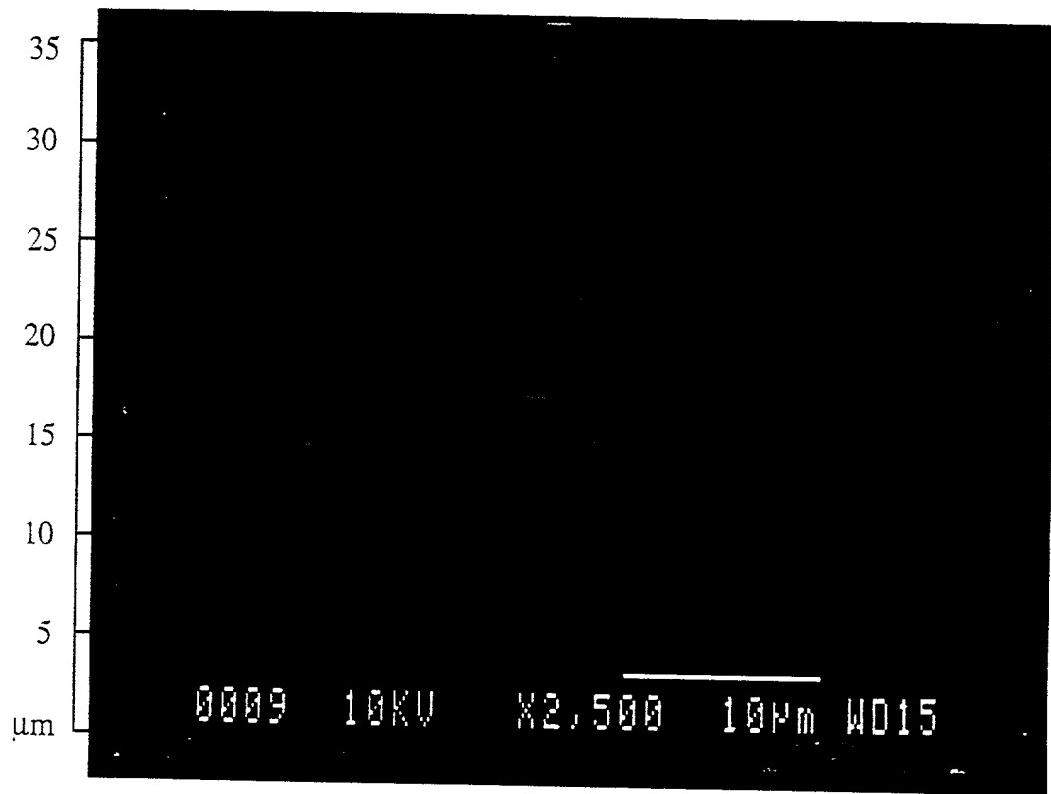


Fig. 14b